
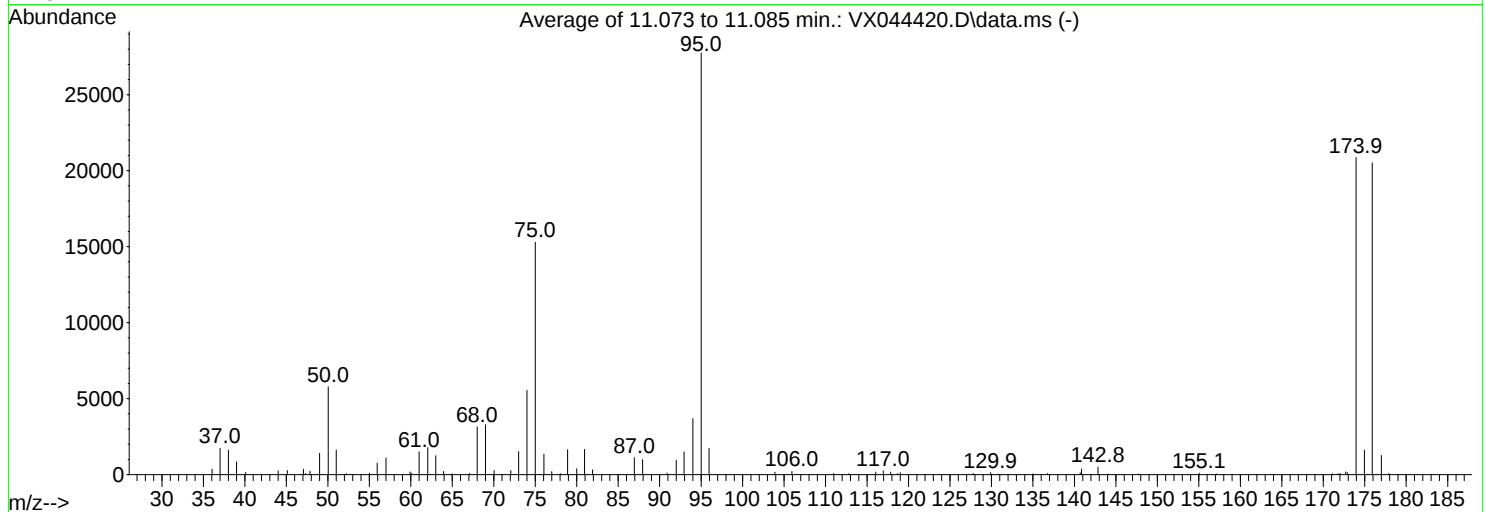


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121924\
Data File : VX044420.D
Acq On : 19 Dec 2024 07:49
Operator : JC/MD
Sample : BFB707
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB707

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis
Last Update : Wed Dec 18 04:40:20 2024

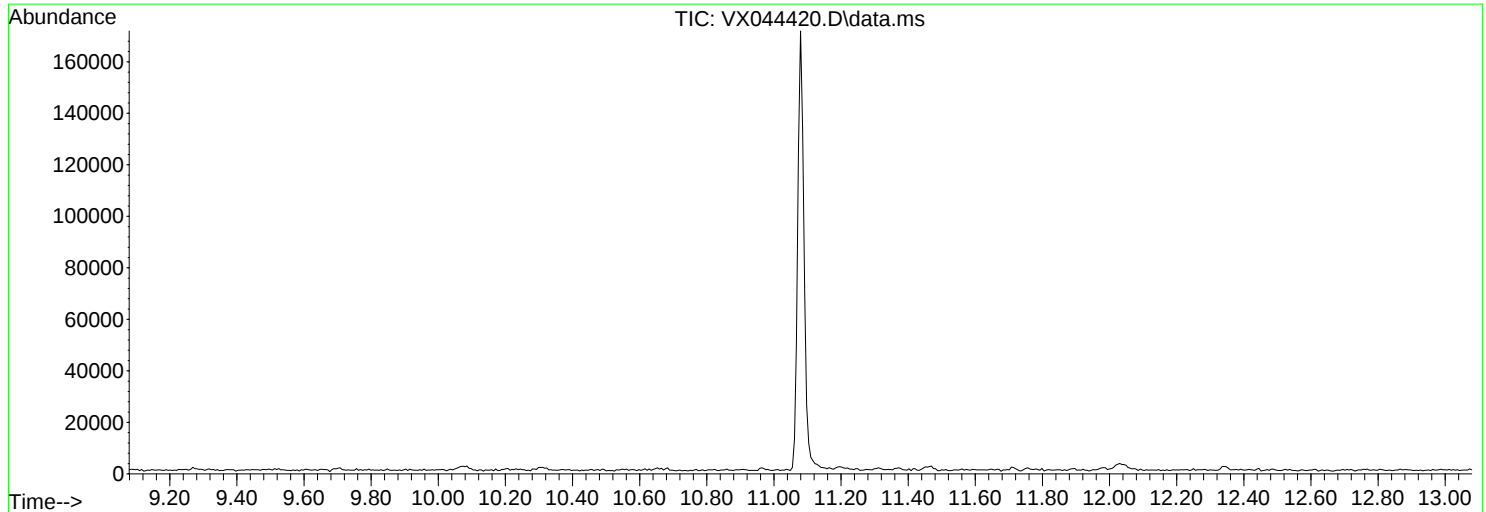

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	5785	PASS
75	95	30	80	55.1	15297	PASS
95	95	100	100	100.0	27755	PASS
96	95	5	9	6.2	1723	PASS
173	174	0.00	2	0.9	184	PASS
174	95	50	120	75.2	20863	PASS
175	174	5	9	7.7	1607	PASS
176	174	95	101	98.4	20519	PASS
177	176	5	9	6.2	1264	PASS

m/z	Abundance
37.00	102.0
37.90	130.0
38.30	168.0
39.00	310.0
39.90	506.0
41.20	103.0
44.10	263.0
90.90	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB707

m/z	Abundance
36.00	328.0
37.00	1620.0
38.00	1637.0
39.00	1064.0
39.90	467.0
41.20	104.0
44.10	557.0
45.10	243.0
47.10	343.0
47.80	245.0
49.00	1412.0
50.00	6249.0
51.00	1730.0
52.20	114.0
55.00	91.0
56.00	630.0
57.00	1029.0
59.90	275.0
61.00	1198.0
62.00	1816.0
63.00	1184.0
63.90	227.0
65.10	60.0
66.90	67.0
68.00	3461.0
69.00	3047.0
70.10	256.0
72.00	342.0
73.00	1072.0
74.00	4967.0
75.00	14205.0
76.00	1338.0
77.00	124.0
78.00	111.0
78.90	1520.0
80.00	419.0
80.90	1554.0
81.90	349.0
87.00	1328.0
88.00	786.0
91.00	74.0
92.00	841.0
92.90	1316.0
94.00	3557.0
95.00	25440.0
96.00	1549.0
103.80	110.0
106.00	216.0
111.00	50.0
112.80	61.0
116.10	173.0
116.90	161.0
118.00	185.0
119.00	129.0
127.80	109.0
129.90	110.0
131.30	57.0
135.00	64.0
136.90	65.0
140.70	336.0
142.80	359.0
144.10	71.0
148.00	63.0
155.00	94.0
172.10	91.0
172.70	212.0
173.90	15046.0
174.90	1171.0
175.90	15684.0
177.00	1097.0
178.00	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB707

m/z	Abundance
36.10	435.0
37.10	2168.0
38.10	2299.0
39.10	1211.0
39.90	511.0
41.00	173.0
43.90	385.0
45.10	394.0
47.00	720.0
47.90	215.0
49.00	1822.0
50.10	6436.0
51.00	2037.0
52.20	97.0
55.00	147.0
56.00	905.0
57.00	1419.0
59.90	253.0
61.00	1760.0
62.10	1989.0
63.00	1406.0
63.90	208.0
64.90	72.0
67.10	140.0
68.00	3779.0
69.00	4029.0
70.00	301.0
72.10	315.0
73.00	2073.0
74.00	6878.0
75.00	18688.0
76.10	1544.0
77.10	253.0
78.10	72.0
78.90	1954.0
80.00	490.0
81.00	1964.0
81.80	411.0
87.00	1090.0
87.90	1282.0
91.00	218.0
92.00	945.0
93.00	1734.0
94.00	4540.0
95.00	33072.0
96.00	2037.0
103.90	177.0
104.90	76.0
105.90	206.0
111.00	85.0
112.80	129.0
116.00	146.0
116.90	244.0
117.80	132.0
118.70	162.0
119.00	154.0
127.80	74.0
129.00	66.0
130.00	173.0
130.80	74.0
135.00	103.0
136.70	89.0
140.90	606.0
142.90	561.0
144.00	52.0
153.60	66.0
155.10	92.0
157.10	79.0
171.20	100.0
172.00	134.0
172.70	341.0
173.90	24440.0
175.00	2140.0
175.90	24944.0
177.00	1319.0
177.90	116.0

Instrument :
MSVOA_X
ClientSampleId :
BFB707

m/z	Abundance
36.10	303.0
37.00	1710.0
38.10	1297.0
39.00	1171.0
40.10	457.0
43.90	617.0
45.10	193.0
47.30	233.0
47.90	237.0
49.00	977.0
50.00	4669.0
51.00	1094.0
55.00	84.0
55.90	729.0
57.00	861.0
60.10	288.0
61.00	1551.0
62.00	1542.0
63.00	1129.0
64.00	198.0
64.90	73.0
67.10	108.0
68.00	2172.0
69.00	2793.0
70.10	263.0
72.00	150.0
73.00	1390.0
74.00	4817.0
75.00	12997.0
76.00	1171.0
76.90	221.0
78.90	1456.0
80.00	267.0
81.00	1473.0
82.00	203.0
83.10	52.0
86.80	966.0
88.00	946.0
90.80	172.0
92.00	1045.0
93.00	1435.0
94.00	2956.0
95.00	24752.0
95.90	1584.0
104.00	193.0
105.90	218.0
106.60	65.0
110.80	77.0
116.00	186.0
117.00	357.0
117.80	191.0
119.00	125.0
127.80	56.0
129.80	132.0
130.80	52.0
136.70	77.0
140.80	499.0
142.90	559.0
147.70	128.0
155.00	115.0
157.10	69.0
171.00	89.0
171.80	178.0
172.90	422.0
174.00	23104.0
175.00	1511.0
175.90	20928.0
177.00	1375.0
177.80	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB707